



TECHNIMOUNT
EMS®

BRACKET PRO SERIE® 22

USER MANUAL



SAFETY AND FLEXIBILITY
WHERE IT MATTERS MOST

Copyrights

Copyright Technimount E.M.S. Holding Inc. is an affiliated company of Technologies CGC Inc. All Rights Reserved. No part of this publication may be reproduced, transmitted, transcribed, backed-up on a retrieval system, translated in any language, modified in any form or by any means, without the written permission of Technimount or its affiliate companies.

Trademarks

Product and medical device manufacturer names are Trademarks™ or Registered Trademarks® of their respective holders.

- Technimount EMS® and Bracket Pro Serie® are registered trademarks of Technologies CGC Inc.
- ZOLL® and M2® are registered trademarks of ZOLL Medical Corporation.
- Oxivir® is a registered trademark of Diversey.

For any issues with your Technimount product, its components, or for any technical questions during the installation, operation, or maintenance, please contact Technical Support at techsupport@technimount.com.

Contact Information

Technimount E.M.S. Holding Inc.

C/O: Regulatory Affairs

3770 Jean Marchand Street, Suite 100-C

Quebec (Quebec) G2C 1Y6

Canada

customerservice@technimount.com

techsupport@technimount.com

legal@technimount.com

www.technimount.com

T + 1 581 700-6613

TF + 1 888 639-2758 (North America)

Table of Contents

Copyrights	ii
Trademarks	ii
Contact Information	ii
1. General Mentions and Considerations	5
..... 1.1. Intended Use	5
..... 1.2. User Competency	5
..... 1.3. Warranties	6
..... 1.3.1. Warranty Policy	6
..... 1.3.2. Limited Warranty	6
..... 1.3.3. International Warranty Clause	6
..... 1.3.4. User Liability	6
..... 1.4. Claims	7
..... 1.4.1. Damaged or Defective Merchandise	7
..... 1.4.2. Return Policy	7
..... 1.4.3. Return of Material Authorization (RMA)	8
..... 1.4.4. Claim Process	8
2. General Safety Guidelines	9
..... 2.1. Symbols and Definitions	9
..... 2.2. Labels	10
..... 2.3. Safety Measures	11
3. Technical Specifications	12
4. Bracket Pro Serie 22 Orientation Diagrams	13
5. Bracket Pro Serie 22 Illustrated Parts	14
6. Operate the Bracket Pro Serie 22	15
..... 6.1. Install the Bracket Pro Serie 22 in a Standard Surface Base	15
..... 6.2. Remove the Bracket Pro Serie 22 from a Standard Surface Base	16
Annex I Clinical Staff Skills Assessment	17
Annex II Unpack the Bracket Pro Serie 22	19
Annex III Prepare the Bracket Pro Serie 22	21
..... Required Installation Time	21
..... Required Tools	21
..... Install the Medical Device in the Support Bracket	21

Annex IV Maintenance	23
..... Maintenance Frequency.....	24
..... Required Tools	24
..... Approved Cleaning Solutions	24
..... Maintenance Plan.....	25
..... Illustrated Inspection Points.....	28
Annex V Replacement Parts/Kits	29

1. General Mentions and Considerations

The Bracket Pro Serie 22 user manual includes detailed product information, standards and guidelines to assist the administrator/manager/supervisor and biomedical technician (or equivalent) with the unpacking, assembling (when indicated) and maintenance of the Technimount product. It also includes specific user-related information to assist trained EMS and clinical personnel with effectively operating the support bracket.

Please read the user manual thoroughly to fully assess, comprehend, then relay its content to EMS and clinical personnel during training, to warn them of any potential danger of its abuse, how to safely use the product and provide a safe environment for patients as well as themselves. Your established internal protocols should be updated to include the Technimount product(s) standards, guidelines, requirements and safety recommendations included within this documentation. The user manual should remain available to users when needed and relayed if the product is subsequently sold.

NOTE : Technimount continually seeks advancements in product design and quality. While the user manual contains the most updated product information available at the time of printing, it may contain minor differences from the current version, including image references. For more information, please contact Technical Support at techsupport@technimount.com.

NOTE : Technimount reserves the right to change part numbers and products without notice. Please contact Customer Service at customerservice@technimount.com to ensure product options and availability.

1.1. Intended Use

The Bracket Pro Serie 22 is designed to aid trained EMS and clinical personnel hold and secure the ZOLL M2 monitor/defibrillator with accessory bags during ground emergency medical services and critical care.

1.2. User Competency

To safely operate the support bracket, EMS and clinical personnel must have the required skill level. Training should be given to EMS and clinical personnel, taking in account the skill level that is necessary to comply with their function and level of interaction with the Bracket Pro Serie 22:

- **Proficient (trained EMS and clinical personnel):** Has received the required training, is sufficiently knowledgeable to safely operate the product and have passed the skills assessment (refer to « Annex I Clinical Staff Skills Assessment » on page 17).

NOTE : Any member of the EMS and clinical personnel who has not received the required training and lacks the knowledge needed to safely operate the support bracket must not use the product.

- **Expert (administrator/manager/supervisor):** Has in-depth knowledge and product comprehension, and is familiar with standards and guidelines. Skilled to train EMS and clinical personnel on how to safely use the product.
- **Advanced (biomedical technician or equivalent):** Has extensive mechanical experience. Skilled to perform the unpacking, assembly, safety checks and condition-based maintenance procedures as detailed in « Annex IV Maintenance » on page 23, basic troubleshooting, upgrade procedures and replacement procedures.

1.3. Warranties

1.3.1. Warranty Policy

This statement constitutes Technimount's entire warranty policy with regards to Technimount products. Technimount makes no other warranty or representation, neither expressed nor implied, except as stated herein. There is no warranty of merchantability or warranty of fitness for any particular purpose. Under no circumstances will Technimount be held liable hereunder for incidental or consequential damages, arising from or in any manner, related to sales or use of any such product.

Technimount E.M.S. Holding Inc. guarantees to the original "Purchaser" of the "Product" with which this "Limited warranty" is included, that the product will be free from "Defects" in workmanship and materials under normal use for a "Warranty period" of one (1) year from the product purchase date by the purchaser. During the warranty period, the product will be repaired or replaced according to the "Limited warranty" without charge to the purchaser for parts or labor. The parts and product may be repaired or replaced with new or refurbished parts or products. Herein this Limited Warranty, "Refurbished" means parts and products which have been returned to the factory, specifically. If the product is repaired or replaced within the warranty period, the greater of the remaining warranty period will apply, or three (3) months from the date of repair or replacement. If the product is repaired or replaced after the warranty period has expired, the warranty period for the repair or replacement will expire three (3) months after the repair or replacement date.

1.3.2. Limited Warranty

Technimount products are intended to retain medical devices in place in the case of single crash impact. Technimount products must not be reused if involved in a single crash impact and must thereafter be replaced. If the end user uses a Technimount product following a single crash impact, it is at the end user's own risk and Technimount will not be held liable.

The limited warranty does not apply to normal wear that could result from normal use. It does not apply when the product or any of its components have been disassembled or repaired by someone not authorized by "Technimount". It does not cover repair or the replacement of any product or part thereof damaged by neglect, misuse, moisture, liquids, exposure to heat, accidents, abuse, and non-compliance with the instructions for installation and use provided with the product. It does not cover physical damage to the surface of the product. The decision to repair, replace or refuse the coverage is final and at the sole discretion of Technimount, without any compensation or obligation from Technimount. The product defined as a "support bracket" or "bracket", used to hold and secure the ZOLL M2 monitor/defibrillator with accessory bags, is specifically designed to fill this requirement. Any other use will void the warranty and Technimount shall not be held liable on any claim if the product has been modified or adapted for use.

1.3.3. International Warranty Clause

This warranty abides by the Canadian domestic policy. Warranty outside Canada may vary by country. Please contact Customer Service at customerservice@technimount.com for more information.

1.3.4. User Liability

The purchaser and administrator are responsible to validate regulations and standards for safety in their region, to comply with applicable safety regulations. Technimount is not responsible to inform the purchaser or the

administrator of any applicable legislation for safety in their area.

The administrator is responsible for providing proper training to any personnel who will install, operate and perform maintenance on Technimount products.

1.4. Claims

1.4.1. Damaged or Defective Merchandise

ICC Regulations require that claims for damaged merchandise must be made with the carrier within fifteen (15) days of the reception date. **Do not** accept damaged merchandise unless such damage is noted on the delivery receipt at the time of reception. Upon prompt notification, Technimount will file a freight claim with the appropriate carrier for damages incurred. Claims are limited in amount to the actual replacement cost. If the claim has not been received by Technimount within the fifteen (15) day period following the date of delivery, or the damage was not noted on the delivery receipt at the time of receipt, the customer will be responsible for the full payment of the original invoice.

Claims for any short or broken merchandise must be made within thirty (30) days of invoicing. For details, refer to the claim process or contact Customer Service at customerservice@technimount.com.

1.4.2. Return Policy

Technimount products may be returned up to sixty (60) days from the reception date, if:

- The received product does not match what was originally ordered.
- The product does not meet the Technimount technical sheet specifications.
- The product is not compatible with the system on which it was intended to be installed on.

To return a Technimount product,

- A Return of Merchandise Authorized (RMA) must be requested and approved by Technimount prior to returning the product.
- Products must be returned undamaged and in its original packaging, appropriately identified with the approved RMA number. Returns will not be approved on a modified or damaged item.
- Charges may apply if the package received is damaged or items are missing.
- Purchaser is responsible for a restocking fee (refer to Table 1).

Table 1: Restocking fees

RESTOCKING FEES	
Prior to thirty (30) days	10%
Prior to forty-five (45) days	25%
Prior to sixty (60) days	30%

For any manufacturing defect, refer to the conditions within the warranty policy or contact Customer Service at customerservice@technimount.com for additional information.

1.4.3. Return of Material Authorization (RMA)

The Technimount Customer Service department is responsible for all merchandise returns and will provide a Return of Merchandise Authorization (RMA) number, upon approval. The RMA must be printed and placed on the returned merchandise. Technimount reserves the right to charge shipping and restocking fees (refer to Table 1 on page 7) for the returned items. Special, modified, or discontinued items are not subject to returns.

1.4.4. Claim Process

Upon reception of the returned merchandise, a thorough inspection will be performed. If the merchandise is compliant with the return policy or it is found that the product is defective, Technimount will take corrective actions and close the claim. If, however, it is found that the product is not defective, but rather misused or abused, the product will not be covered by the warranty. Details of our findings and conclusions will be provided shortly thereafter. To submit a claim, contact Customer Service at customerservice@technimount.com to obtain a Return of Material Authorization (RMA) form and return instructions.

2. General Safety Guidelines

Always read and abide by all the safety guidelines identified within this document. Pictograms, safety symbols and labels are used to alert the user to a potentially hazardous situation, which, if not avoided, may result in minor or moderate injury to the patients or EMS and clinical personnel, or damage to the product. This includes the special care necessary for the safe and effective use of the Technimount product to avoid damage that may occur from use or misuse. The terms "Warning" and "Caution" herein carry special meaning and should be carefully reviewed.

WARNING – Indicates a hazardous situation that, if not avoided, could result in death or serious injury.

CAUTION – Indicates a hazardous situation that, if not avoided, could result in minor or moderate injury.

2.1. Symbols and Definitions



WARNING – Risk of Injury

Indicates when a misuse of the Technimount product could result in injuries to the patients or EMS and clinical personnel, or damage to the product.



CAUTION – Safe Practice

Alerts the reader to pay special attention to the recommendations and methods outlining how to safely operate the product to minimize risks to the patients, EMS and clinical personnel and the product.



CAUTION – Safe Handling and Operation

Alerts the reader to pay special attention to the recommendations for safe use of the product, and of potentially hazardous situations that could result in minor injuries to the patients or EMS and clinical personnel. This includes the special care necessary for the safe and effective use of the product to avoid damage that may occur from use or misuse.



CAUTION – Safe Working Load (SWL)/Load Balance

Indicates the total maximum charge for a safe use of the product.




CAUTION – Follow Instructions for Use

Call for action. Reminds the reader to consult the user manual for information.

2.2. Labels

Labelling on the surface of the Technimount product, quickly identify potential risks and provides information to the user. A manufacturing label, including the serial number and safe working load label (Figure 1), can be seen on the Technimount product.

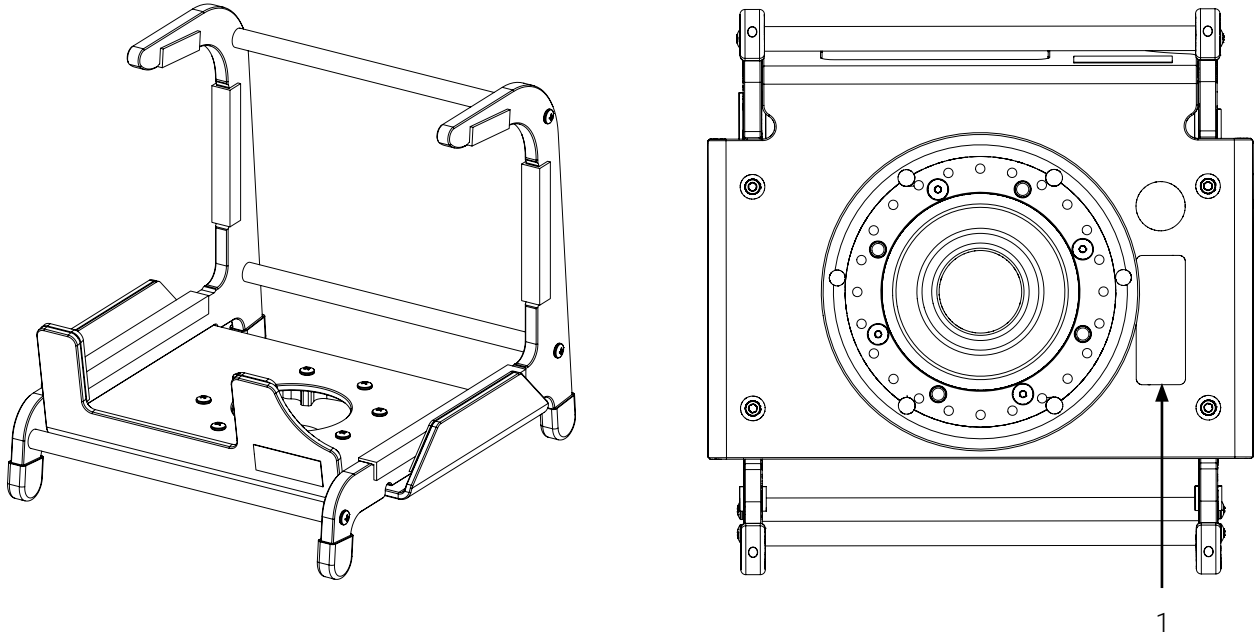

1. Manufacturing label

Figure 1: Location of the manufacturing label (bottom of the bracket)

2.3. Safety Measures

Carefully read all the safety measures herein before operating the Technimount product, relay to EMS and clinical personnel during training, and include in your established internal protocols.

More specific safety measures intended for biomedical technicians (or equivalent) relating to the safety checks and conditioned-based maintenance can be found in « Annex IV Maintenance » on page 23.



WARNING – Risk of Injury

- **Do not** use the support bracket if the bottom plate screws are loose or missing, to prevent undue risk to the medical device, patients, and EMS and clinical personnel.
- Always use the Bracket Pro Serie 22 support bracket as it was intended, using only the compatible medical device and accessories. Improper use of the Technimount product may cause unpredictable functioning resulting in injury to the patients or EMS and clinical personnel. Refer to the « Technical Specifications » on page 12 for compatibilities.
- If any serious incident occurs with the support bracket, immediately stop using the product, report this incident to Technical Support at technicalsupport@technimount.com and the applicable regulatory agency.



CAUTION – Safe Practice

- Always pay close attention to the condition of the safety mechanisms of the support bracket to avoid risks of damage, equipment falling, or injuries to the patients or EMS and clinical personnel.
- Practice safely operating the support bracket until the manipulations have been perfected, before use with patients. Improper use of a Technimount product may damage it or cause injury to the patients or EMS and clinical personnel.
- Regulations and standards for safety are the sole responsibility of the end user. Ensure that the installation specifications meet the local and regional compliance requirements before use.
- Refer to your established internal protocols and the user documentation provided with the medical device for the safety guidelines and safe use.



CAUTION – Safe Handling and Operation

- Always ensure that the monitor/defibrillator is secured in the support bracket before it is moved to avoid risks of damage, equipment falling, or injuries to the patients or EMS and clinical personnel.
- Always pay close attention not to wedge the power cords or cables during the installation or the removal of the support bracket. Refer to your established internal protocols for the safety guidelines and safe use with the medical device.



CAUTION – Safe Working Load (SWL)/Load Balance

Do not overload the support bracket to avoid tipping incidents or risks of collapsing. The total Safe Working Load (SWL) is 22 lb (9.97 kg).



CAUTION – Follow the Instruction for Use


- Always read and abide by all the safety guidelines identified, as well as follow instructions provided within the user manual of the Bracket Pro Serie 22.
- The Bracket Pro Serie 22 is specifically designed to be used with the ZOLL M2 monitor/defibrillator. Refer to the user documentation of the medical device for the safety guidelines and safe use.

3. Technical Specifications


Product Name	Bracket Pro Serie® 22
Description	Support bracket designed to aid trained EMS and clinical personnel hold and secure the ZOLL® M2® monitor/defibrillator with accessory bags
Product Code	150-10-M2Z
Operating Environment	<ul style="list-style-type: none"> - EMS/CCT (ground) - Hospital/Clinic
Compliance	Tested in compliance with SAE J3043 and AMD-028
Expected Service Life	5 year
Compatible Stretcher	N/A
Compatible Mounting System	<ul style="list-style-type: none"> - Standard Surface Base - Extended Surface Base - Universal Mounting Base
Compatible Medical Devices/ Accessories	ZOLL® M2® monitor/defibrillator with accessory bags
Dimensions (W X D X H)	11.07 in. X 11.48 in. X 10.47 in. (28.12 cm X 29.16 cm X 26.60 cm)
Weight	5.41 lb (2.46 kg)
Composition	Aluminum, rubber
Total Safe Working Load (SWL)	22 lb (9.97 kg)
Operating Temperature	- 31° F to 113° F (- 35° C to 45° C)
Approved Cleaning Solutions	<ul style="list-style-type: none"> - Oxivir®, 5% Hydrogen Peroxide with Peracetic Acid (AHP) - TNT-100, 5% Quaternary Ammonium Compound - Spectro-Sept, 5% Ethyl Alcohol - Spectrol, 5% EDTA salt
Options	N/A

4. Bracket Pro Serie 22 Orientation Diagrams

NOTE : The orientations referenced herein are from the EMS and clinical personnel standpoint, when facing the support bracket.

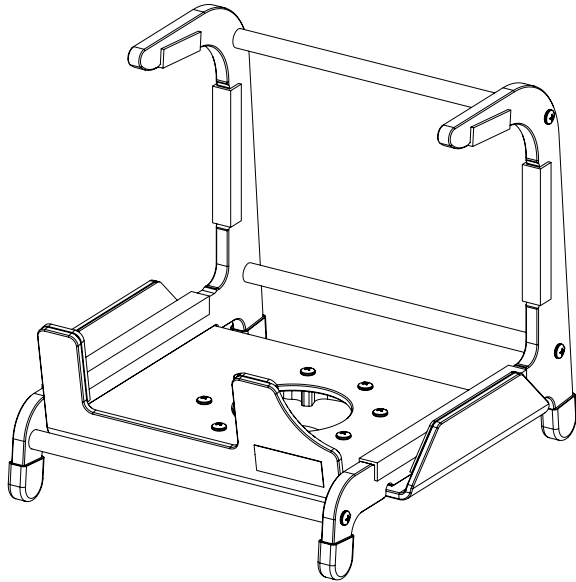

Front of the support bracket

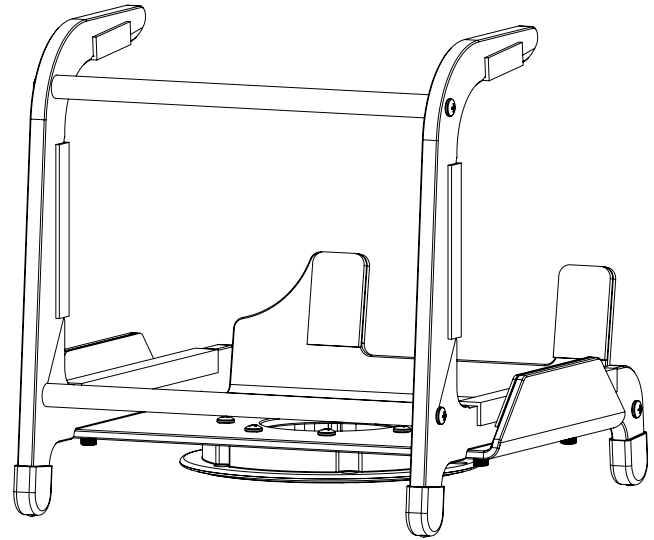

Back of the support bracket

Figure 2: Orientation diagram of the Bracket Pro Serie 22

5. Bracket Pro Serie 22 Illustrated Parts

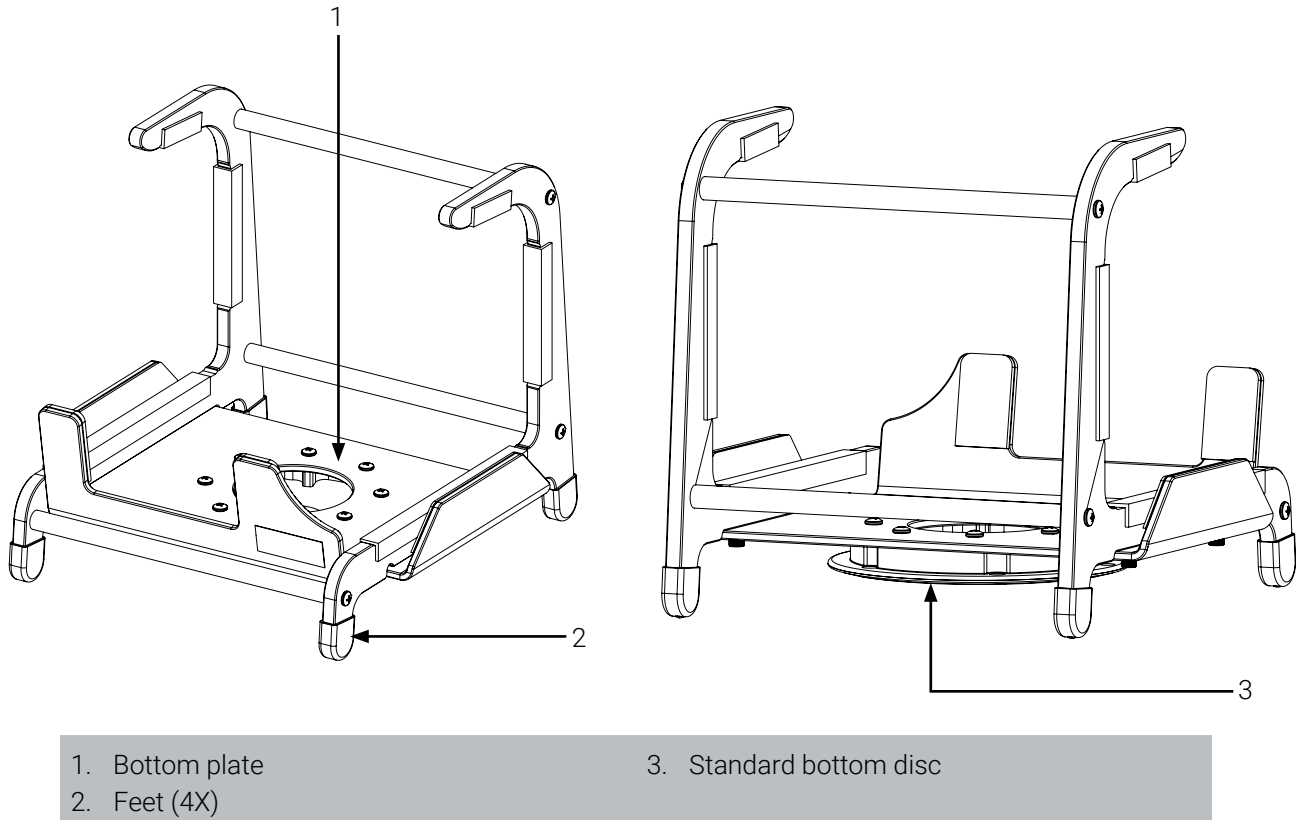


Figure 3: Components of the Bracket Pro Serie 22

6. Operate the Bracket Pro Serie 22

The content in this section is intended for EMS and clinical personnel who are proficient, have received the required training and passed the skills assessment, therefore sufficiently knowledgeable to safely operate the support bracket.

6.1. Install the Bracket Pro Serie 22 in a Standard Surface Base

1. Align and insert the disc of the support bracket in the Standard Surface Base (Figure 4 A), paying close attention not to wedge the cables of the medical device.
2. Push the support bracket all the way back in the base until it is locked (Figure 4 B).

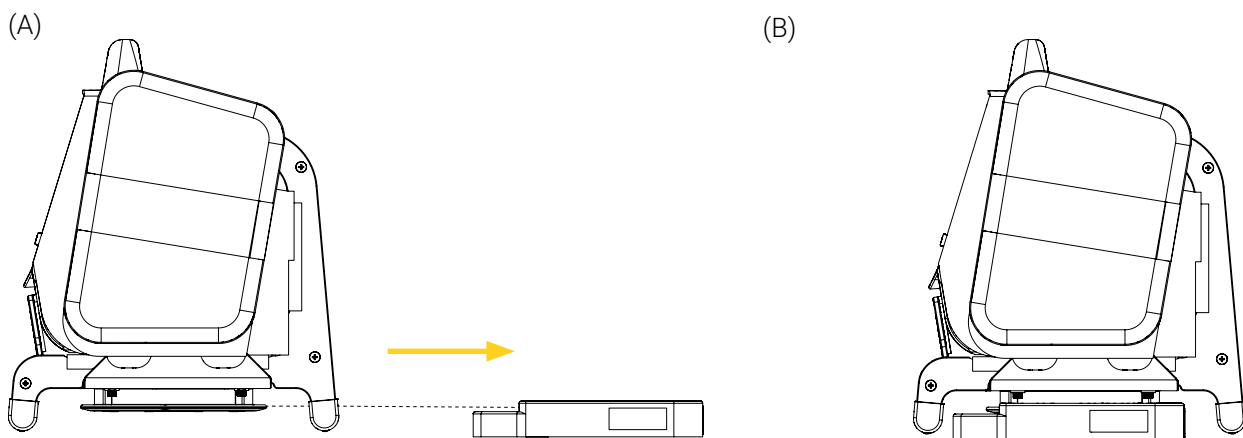


Figure 4: Installing the support bracket in a Standard Surface Base

3. Move the support bracket back and forth a few times to ensure it is locked and secured in the Standard Surface Base. If the disc stays in the base after the verification, the bracket is locked and secured.
4. Turn the support bracket clockwise or counterclockwise to the desired position (Figure 5).

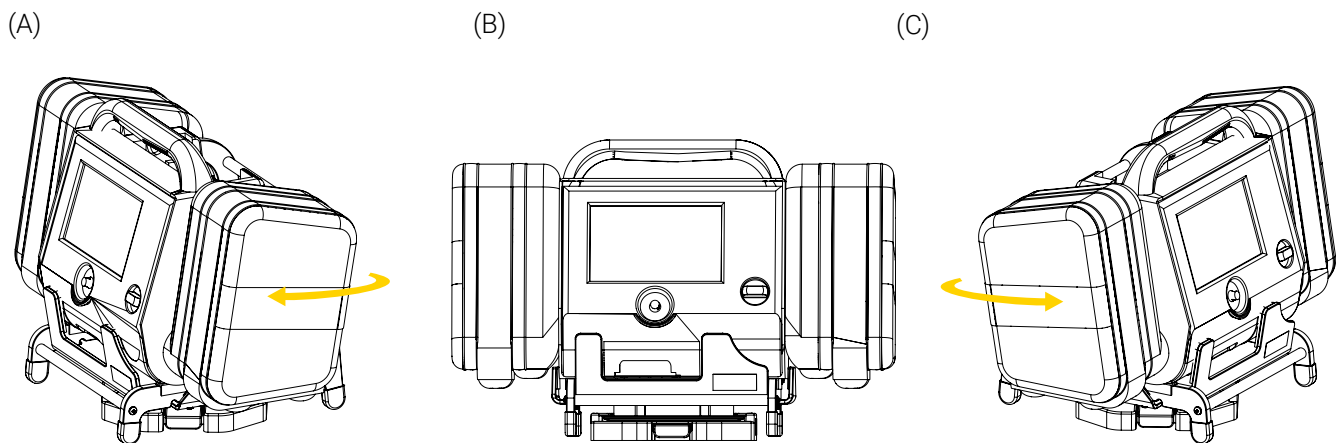


Figure 5: Operating the support bracket in the Standard Surface Base

The installation of the Bracket Pro Serie 22 in a Standard Surface Base is complete.

6.2. Remove the Bracket Pro Serie 22 from a Standard Surface Base

1. Press and hold the quick release button of the Standard Surface Base (Figure 6 A), then pull the support bracket out of the base (Figure 6 B).

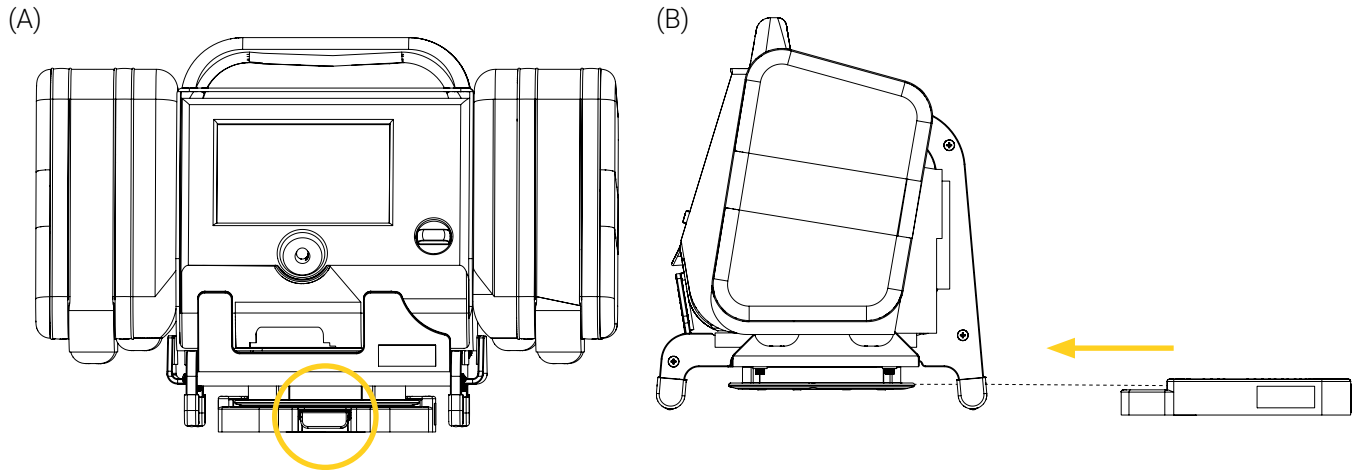


Figure 6: Removing the support bracket from a Standard Surface Base

2. Set aside the support bracket aside on a flat and clean surface, or store as per your established internal protocols.

The removal of the Bracket Pro Serie 22 from a Standard Surface Base is complete.

Annex I Clinical Staff Skills Assessment

Following training, a skills assessment should be given to each member of the clinical staff to ensure they have fully comprehended the labelling, warnings and cautions, potential risks, safe practices and proper operating procedures needed to safely and effectively use the support bracket. Consider adding the following to your internal training protocols.

Trainee name: _____ Unit: _____

Assessor name: _____ Date: _____

CLINICAL STAFF SKILLS ASSESSMENT

SKILL CRITERIA

PASSED
FAILED

Labelling

- Able to identify meaning and potential risks associated with the different safety labels:
 - Safe Working Load (SWL)

Safety Measures

- Knows **not to** use the Bracket Pro Serie 22 if the bottom plate screws are loose or missing.
- Knows to always use the Bracket Pro Serie 22 support bracket as it was intended, using only the compatible medical device and accessories.
- Knows to always pay close attention to the condition of the safety mechanisms of the support bracket.
- Knows to always ensure that the monitor/defibrillator is secured in the support bracket before it is moved.
- Knows to always pay close attention not to wedge the power cords or cables during the installation or the removal of the support bracket.
- Knows **not to** overload the support bracket.
- Knows to always read and abide by all the safety guidelines identified, as well as follow instructions provided within the user manual of the Bracket Pro Serie 22.

Operation

- Able to install/remove a support bracket on/from the Standard Surface Base.
- Able to operate a support bracket on the Standard Surface Base.
- Has practiced safely operating the support bracket, has perfected the manipulations and has acquired the required skill level to safely use with patient.

Annex II Unpack the Bracket Pro Serie 22

Unpacking should be reserved for biomedical technicians (or equivalent) who have extensive mechanical experience, and advanced skill level.

1. Inspect the shipping box(es) for signs of damage before accepting shipment. Take pictures and report them promptly if applicable.
2. Move the shipping box(es) to the location of the installation.
3. Open the shipping box(es).
4. Unpack the box(es) and ensure that all shipping and packaging materials have been properly removed, prior to installation.

NOTE : Keep all packaging material for future use.

5. Identify all the components and hardware included for the installation if applicable, then set them aside. Refer to Annex III on page 21 for the required parts.
6. Inspect the items for signs of damage. Take pictures and report them promptly when applicable.

Annex III Prepare the Bracket Pro Serie 22

The content in this section is intended for biomedical technicians (or equivalent) who have extensive mechanical experience, and advanced skill level and have read the « Safety Measures » on page 11.

Required Installation Time

10 minutes

Required Tools

- Hex key 5/32 in.
- Medium strength thread lock adhesive (🔩)

Install the Medical Device in the Support Bracket

1. Lay the support bracket on it's back on a clean and flat surface to facilitate the installation.
2. Unscrew and remove the bottom plate using a hex key 5/32 in. (Figure 7), then set it aside with it's hardware temporarily.

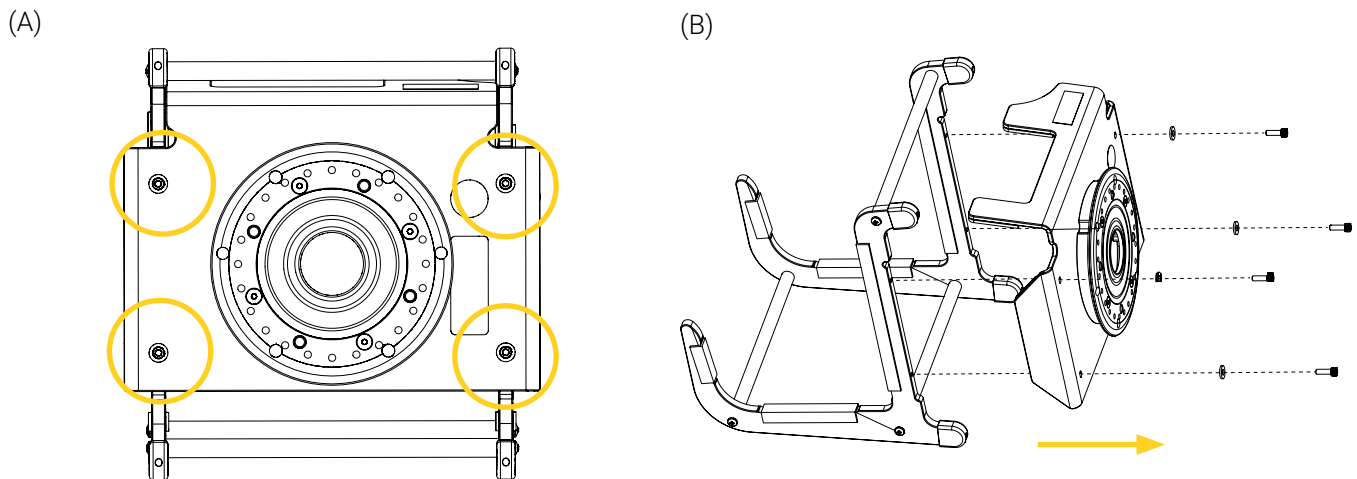


Figure 7: Removing the bottom plate

3. Insert and set the medical device on its back in the support bracket (Figure 8).

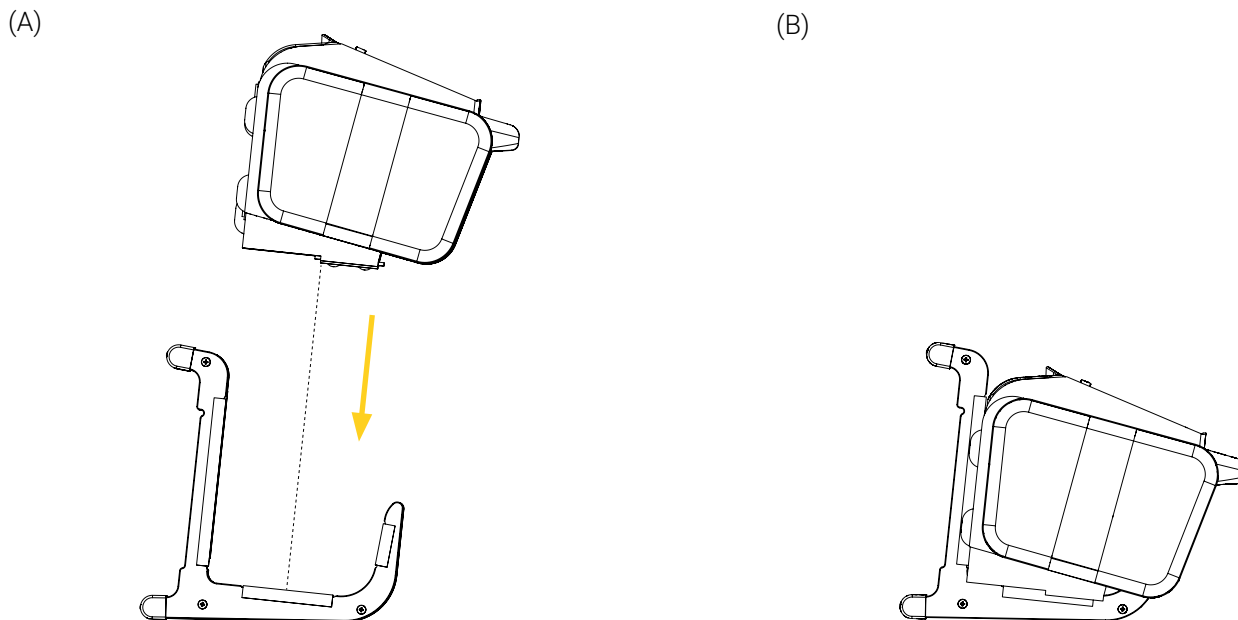


Figure 8: Installing the medical device in the support bracket

4. Reinstall the bottom plate on the support bracket, using the four (4) screws coated with medium strength thread lock adhesive, four (4) washers and a hex key 5/32 in. (Figure 9 A).
5. Ensure that the four (4) screws of the bottom plate are sufficiently tightened. If not, tighten using a hex key 5/32 in.
6. Flip the support bracket on its feet (Figure 9 B).

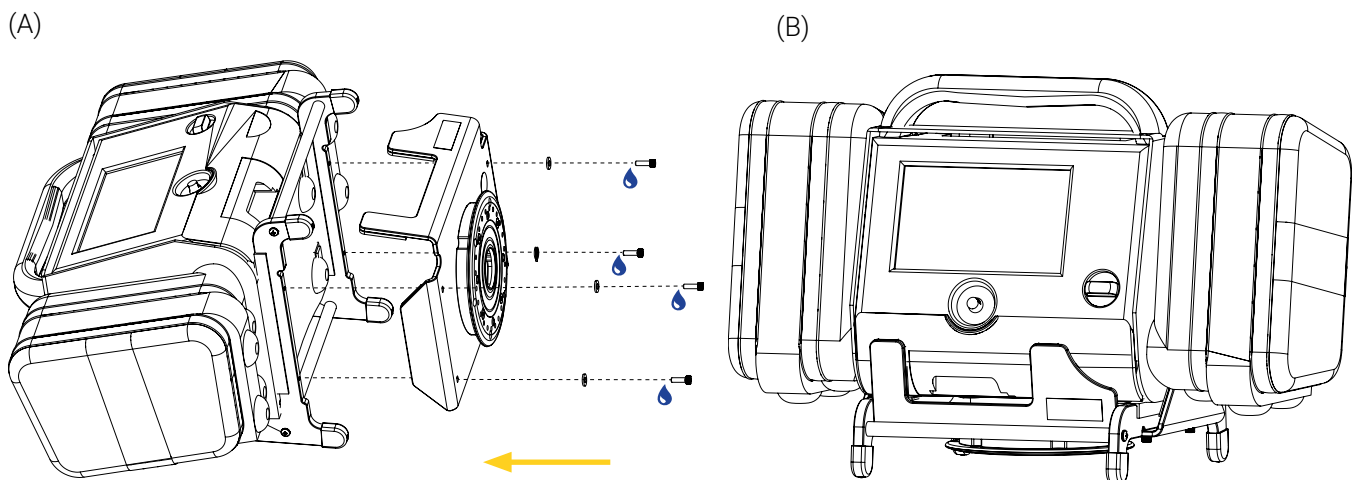


Figure 9: Medical device installed in the support bracket

7. Move the medical device back and forth a few times to ensure it is secured in the support bracket. If it does not move after the verification, it is secured.

The installation of the medical device in the Bracket Pro Serie 22 is complete.

Annex IV Maintenance

Safety checks and condition-based maintenance should be carried out by biomedical technicians (or equivalent) who have extensive mechanical experience, and advanced skill level and have read all the « Safety Measures » on page 11, and the maintenance specific safety measures listed below.

Factors such as weather, environment, geographical location and individual usage will necessitate different needs. For the maintenance of the Bracket Pro Serie 22, follow the guidelines listed herein and in accordance with your service's current maintenance practices and established internal protocols. Please contact Technical Support at techsupport@technimount.com for replacement parts or repair related issues, if needed.



WARNING – General Warning

- **Do not** perform safety checks or condition-based maintenance before having read the entire content of the user manual, gained in-depth knowledge and product comprehension, and familiarized yourself with the standards and guidelines.
- Safety checks and a condition-based maintenance plan are required and should be established for all Technimount products.
- Perform the safety checks and maintenance operations as described herein. Failing to follow the recommended maintenance plan or its guidelines could cause premature damage to the product.
- Use only Technimount parts, maintenance procedures, cleaning solutions and lubricants, as described herein. Using unapproved modified parts or procedures for the maintenance of the Technimount product may cause the system to be unstable and could cause injury to the patients or EMS and clinical personnel and void the product warranty.
- Replace damaged or worn-out parts if past their expected service life or when damaged (refer to « Annex V Replacement Parts/Kits » on page 29). Recycle damaged parts or dispose according to the environmental laws that apply to your jurisdiction and consult the Safety Data Sheets (SDS).



CAUTION – Safe Handling and Operation

- **Do not** use unauthorized, unapproved or untested cleaning products or disinfectants. Performing condition-based maintenance using untested cleaning product could damage the surface of your Technimount product and void its warranty. Technimount will not be held liable for damages resulting from the use of an unauthorized, unapproved or untested cleaning product.
- **Do not** use powered tools to screw the hardware during installation, as there is a potential risk of damage to the threads.
- **Do not** steam clean or use ultrasonic cleaners on the system or any of its components.
- **Do not** immerse the metal parts/components in water.
- To spot clean, the maximum water temperature should not exceed 180° F/82° C. The maximum water pressure should not exceed 1500 psi/103.5 BAR. If using a high pressure washer, the pressure nozzle must be kept a minimum of 24 in. (61 cm) from the unit.
- When cleaning, always use appropriate Personal Protection Equipment (PPE) based on established protocols (e.g., gloves, eyewear, etc.).

**CAUTION – Corrosion**

- Always rinse and dry the support bracket properly after using cleaning products. Certain types of cleaners may leave a corrosive residue on the surface of the product and could cause the premature corrosion of critical components. Refer to the product Safety Data Sheets (SDS) for chemical information or handling, storage and emergency measures in case of accident.
- Dispose of corrosive wastes according to the environmental laws that apply to your jurisdiction and consult the Safety Data Sheets (SDS).

**CAUTION – Follow Instructions for Use**

Always read and abide by all the safety guidelines identified, as well as follow instructions provided by the manufacturer of the cleaning product.

Maintenance Frequency

- Safety checks and the condition-based maintenance should be performed minimally every month or as frequently needed, to prolong the longevity of the support bracket in optimal conditions.
- Decontaminate the support bracket as recommended in your established internal protocols, as well as the regulations and standards in virtue of the infection prevention and control procedures.

Required Tools

- Clean dry cloths
- Soft brush
- Pressure washer
- Cleaning solutions
- Hex key 5/32 in.
- Medium strength thread lock adhesive (🔹)

Approved Cleaning Solutions

- Oxivir, 5% Hydrogen Peroxide with Peracetic Acid (AHP)
- TNT-100, 5% Quaternary Ammonium Compound
- Spectro-Sept, 5% Ethyl Alcohol
- Spectrol, 5% EDTA salt

Maintenance Plan

NOTE : In case of a non-conformity, stop using the product and contact Technical Support at techsupport@technimount.com immediately for a remedial action plan.

NOTE : Always keep records of your maintenance activities and immediately remove defective or expired products from your inventory.

MAINTENANCE PLAN	COMPLIANT	
SAFETY CHECKS	YES	NO

Bracket Pro Serie 22 (Figure 10)

- Visually inspect all the components of the support bracket to ensure there is no damage or chemical attack, that the hardware is in good condition and there are no loose screws:
 - Bottom plate.
 - Feet (4X).
 - Standard bottom disc. Refer to the user manual.
- If there is damage to the components, remove the product from circulation and contact Technical Support immediately for a remedial action plan.
- If there are traces of chemical attack, follow the conditioned-based maintenance herein.
- If the hardware is not in good condition, replace it. Contact Technical Support if needed.
- If the hardware is loose, tighten using a hex key 5/32 in.
 - NOTE :** Add medium strength thread lock adhesive when tightening the four (4) screws of the bottom plate
- Insert/remove the standard bottom disc of the support bracket in/from the Standard Surface Base a few times to ensure proper functioning of the locking mechanism of the base. The disc of the support bracket should be easily inserted and locked in position after the click sound, and easily removed when using the quick release button. If not, stop using the product and contact Technical Support for a remedial action plan.

CONDITION-BASED MAINTENANCE**YES NO**

Following the safety checks,

Clean the Bracket Pro Serie 22

1. Remove the excess dirt using a clean cloth, if needed.
2. Remove the contaminants using a pressure washer or as recommended in your established internal protocols and control procedures.
3. Clean using a cloth and cleaning solution.
4. Spot clean stains by applying the solution directly on the stain and let sit on the surface, if needed.

NOTE : Avoid over saturation and ensure that the product does not sit on the surface of the support bracket longer than recommended by the cleaner's manufacturer.

5. Thoroughly rinse the solution with a clean cloth dampened with lukewarm water, then dry all the components using a clean cloth before returning to service.

Comments and observations following the Safety Checks and Condition-Based Maintenance:

Maintenance plan completed on (dd/mm/yyyy):

Maintenance plan completed by:

Illustrated Inspection Points

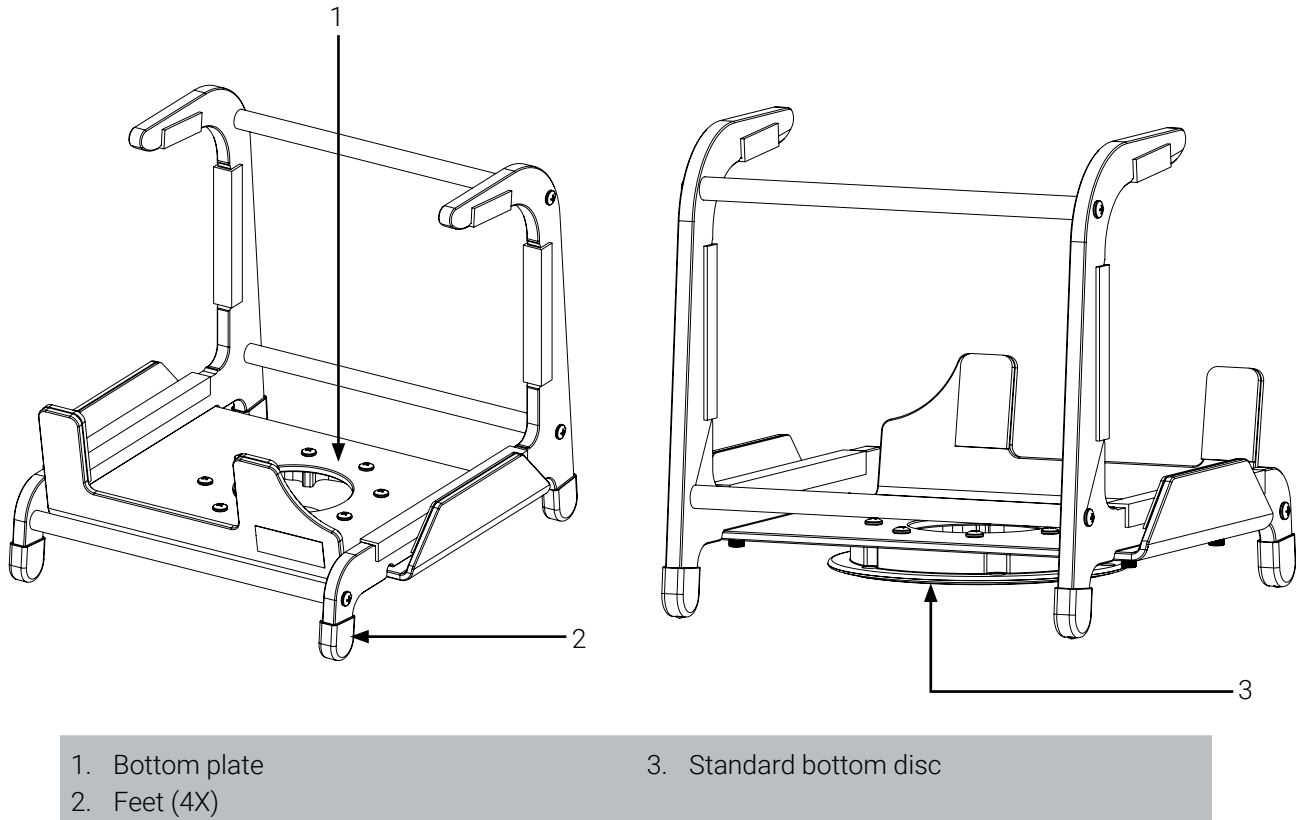


Figure 10: Illustrated inspection points

Annex V Replacement Parts/Kits

Technimount reserves the right to change part numbers and products without notice. Please contact Customer Service at customerservice@technimount.com to ensure product options and availability, or Technical Support at techsupport@technimount.com for replacement parts/kits or repair related issues.

PART/KIT NUMBER	PART/KIT DESCRIPTION
9013-10-M2Z	Rubber feet (4X)
9014-10-M2Z	Hardware (4X)



TECHNIMOUNT
EMS[®]

SAFETY AND FLEXIBILITY
WHERE IT MATTERS MOST