

BRACKET PRO SERIE® 120-GR3 USER GUIDE



Copyright

Copyright 2023 Technimount E.M.S. Holding Inc. (Technimount), an affiliated company of Technologies CGC Inc. All Rights Reserved. No part of this publication may be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any language in any form or by any means without the written permission of Technimount or its affiliate companies.

Trademark Attributions:

Bracket Pro Serie[®], Technimount EMS[™] are registered Trademarks of Technologies CGC Inc. SIGMA Spectrum[®] is a registered trademark from Baxter.

In order to ensure continuous improvements to our products and services, we invite you to communicate your comments to Customer Service at customerservice@technimount.com.

NOTE:

Technimount E.M.S. Holding Inc. does not have a commercial relationship with Baxter.

OFFICE ADDRESS

TECHNIMOUNT E.M.S. HOLDING INC. 3770 Jean Marchand Street, Suite 100-C Quebec (QC) G2C 1Y6 Canada

info@technimount.com www.technimount.com T + 1 581.700.6613 TF + 1 888.639.2758

NOTE:

For any issues with your Technimount product, its components, or for any technical questions during the installation or maintenance, please send an e-mail to techsupport@technimount.com.

Please have the serial number of your Technimount product available (as shown in the figure below) when calling Technimount Customer Service or Technical Support. Include the serial number in all written communications.

SERIAL NUMBER LOCATION BOTTOM VIEW

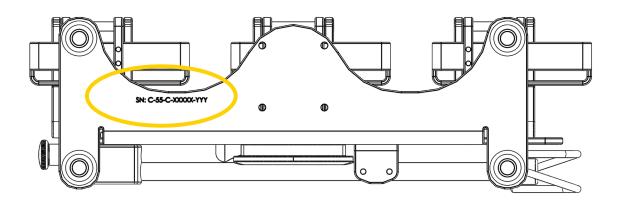


TABLE OF CONTENTS

COPYRIGHT	
CONTACT INFORMATION	
INTRODUCTION	6
Purpose of the Document	6
Product Description	6
Intended Use of the Product	6
Mounting Options for the Bracket Pro Serie [®] 120-GR3	7
Symbols and Definitions	8
Warning / Caution	9
Product Illustrations Bracket Pro Serie 120-GR3	10
FRONT VIEW BACK VIEW	
TECHNICAL SPECIFICATIONS	
NOTICE	-
SUMMARY OF SAFETY PRECAUTIONS	
WARNING/CAUTION/NOTE	
INSTALLATION GUIDE	
Removing the Packaging for Installation	
Tools Required for Installation	
List of Materials	
Installation of the Baxter Pumps onto the Bracket	,
Installation of the IV Pole	5
MOUNTING SYSTEM PART NUMBERS	
Kits and Other Options	
MAINTENANCE GUIDE	
Cleaning the Bracket System	
Cleaning Process Cleaning Solutions	
REMOVAL OF IODINE COMPOUNDS	
Preventive Maintenance	
Inspection Process and Schedule	
MAINTENANCE PLAN	23
Inspection and Maintenance Log	
Training Log	
Replacement Parts	
WARRANTY	
WARRANTY POLICY	
Limited Responsibility and Warranty	27
International Warranty Clause	27
Return Policy	
Prior to 30 Days	
PRIOR 45 DAYS	
Prior 60 Days	28

	Return Authorization	28
	Damaged Merchandise	29
	CLAIM PROCESS	29
	Required Information	29
	FINDINGS AND CONCLUSION	29
	Questions about our Policy	29
SAI	E CERTIFICATION	30

PURPOSE OF THE DOCUMENT

This User Guide is designed to assist you with the installation, operation and maintenance of the Technimount Bracket Pro Serie 120-GR3 Technimount Bracket Pro Serie 120-GR3 for the SIGMA Spectrum Infusion System from Baxter[®].


PRODUCT DESCRIPTION

The Bracket Pro Serie 120-GR3 is a complete mounting system for Baxter SIGMA Spectrum Infusion System on cots /stretchers. It can fit any ground ambulance configurations in North American and European markets. It is designed to securely support and transport up to three SIGMA Spectrum Infusion Systems in pre-hospital and hospital environments. When used in emergency vehicles, the Bracket Pro Serie 120-GR3 can be positioned on Technimount's Safety MD-Transporter. These solutions provide a higher flexibility for different EMS / CCT protocols and applications. This mounting system is compatible with Technimount's products.

INTENDED USE OF THE PRODUCT

The Bracket Pro Serie 120-GR3 is a mounting solution to securely transport up to three SIGMA Spectrum Infusion Systems during intra and inter-hospital transport. It is designed to be installed on the equipment as described in this user guide. This equipment is for medical technicians who have received the appropriate training necessary to operate the equipment in the field according to its intended use as outlined in this user guide. Please read this User Guide thoroughly before using this equipment. To ensure the safe operation of this equipment, it is recommended to train emergency medical personnel prior to use.

MOUNTING OPTIONS FOR THE BRACKET PRO SERIE® 120-GR3

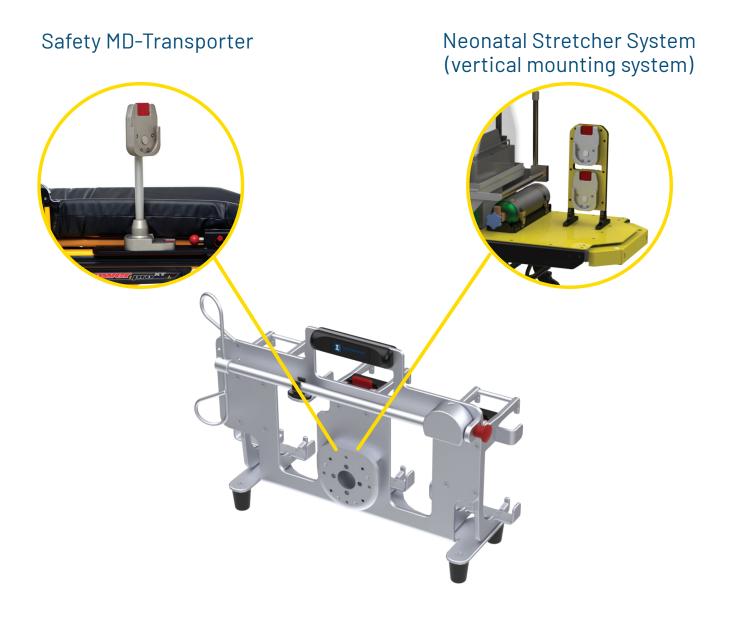

SYMBOLS AND DEFINITIONS

<u>SYMBOL</u>	DEFINITION	
	Alerts the reader of a potentially hazardous situation, which, if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other property. This includes the special care necessary for the safe and effective use of the device and avoid damage that may occur from use or misuse.	
	Indicates the total maximum charge for a safe use of equipment.	
NOTE	Provides supplemental information.	

WARNING / CAUTION


The term Warning, Caution, or note carry special meaning and should be carefully reviewed.

<u>SYMBOL</u>	DEFINITION
	WARNING Indicates a hazardous situation that, if not avoided, could result in death or serious injury.
	CAUTION Indicates a hazardous situation that, if not avoided, could result in minor or moderate injury.

PRODUCT ILLUSTRATIONS

BRACKET PRO SERIE 120-GR3


Front View

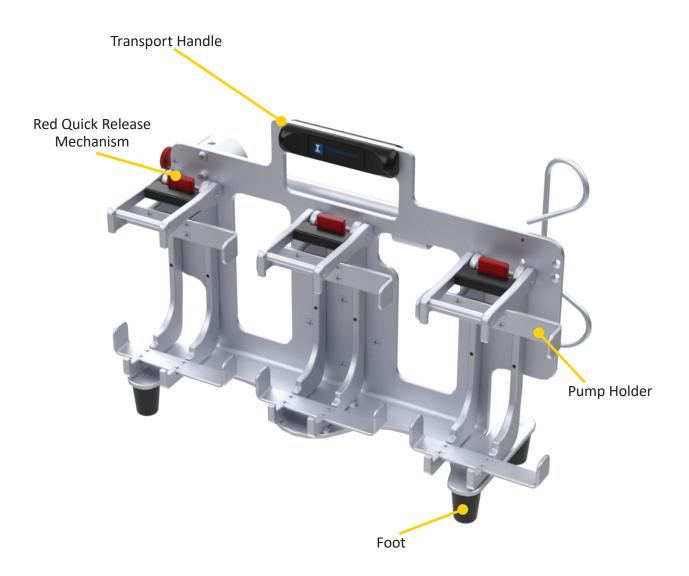

PRODUCT ILLUSTRATIONS (CONTINUED)

BRACKET PRO SERIE 120-GR3 (CONTINUED)

Back View

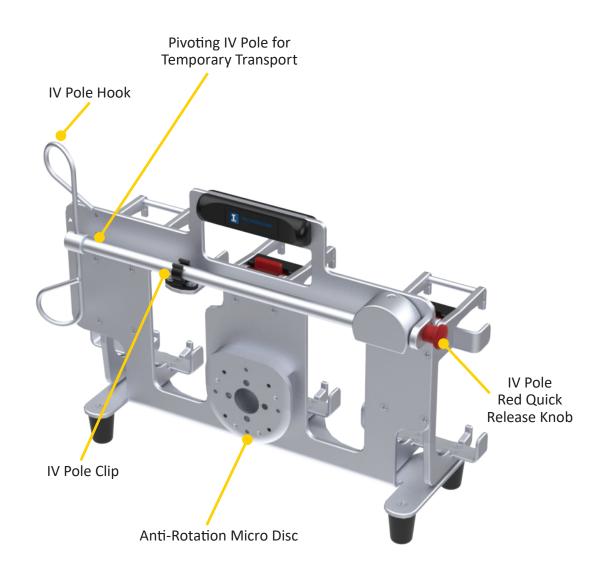

TECHNICAL SPECIFICATIONS

Product Name	Bracket Pro Serie [®] 120-GR3		
Product Description	Bracket mounting solution to securely transport up to three SIGMA Spectrum Infusion Systems during intra and inter-hospital transport.		
Compatibility of Medical Device*	Baxter® SIGMA Spectrum Infusion System		
Environment of Usage	EMS / CCT (Ground) – Hospital / Clinic, Military		
Product Section Material	Main assembly: Aluminum 6061-T6		
	 Anti-Rotation Micro Disc: Aluminum 6061-T6 		
	IV Pole: Aluminum 6061-T6		
	IV Pole Hooks: Stainless Steel		
Product Finish	Main assembly: silver anodized finish		
	Anti-Rotation Micro Disc: silver anodized finish		
	IV Pole: silver anodized finish		
Temperature of Usage	- 31° F to 113° F (- 35° C to 45° C)		
	Tested in compliance with:		
Certification	• SAE J3043		
	• AMD 028		
Installation	Device retained on main assembly with Red Quick Release Mechansim		
Attachment Options	Anti-Rotation Micro Disc		
Transportation Compatibility System	Compatible with Technimount's:		
	Safety MD-Transporter (vertical)		
	Vertical Mounting System		
Features	Robust mounting solution for EMS/CCT		
	 Access to all connectors and accessories 		
	Quick Release Mechanism to easily insert and remove the pumps		
Physical Overall Dimensions (L x D x H)	16.05 in. x 5 in. x 10.7 in. (40.77 cm x 12.7 cm x 27.18 cm)		
Weight	5.07 lbs (2.3 kg)		
Part Number	1500-10-BXSGM-GR3		
Other Models and Configuration Options	Contact Technimount EMS for more information or configuration options at customerservice@technimount.com		

* Product and medical equipment manufacturer names are Trademarks[™] or Registered Trademarks[®] of their respective holders. Technimount does not have a commercial relationship with these medical equipment manufactures.

NOTICE

The Bracket Pro Serie 120-GR3 is designed to comply with the essential requirements and other relevant provisions of SAE J3043 and AMD 028. For more information, please contact Customer Service at customerservice@technimount. com.

TECHNIMOUNT E.M.S. HOLDING INC.

C/O: Regulatory Affairs 3770 Jean Marchand Street, Suite 100-C Quebec (QC) G2C 1Y6 Canada T + 1 581.700.6613 TF + 1 888.639.2758 legal@technimount.com technimount.com



The end user and administrator are responsible to validate regulations and standards for safety in their region, in to comply with applicable safety regulations. Technimount is not responsible to inform the end user or the administrator of any applicable legislation for safety in their area.

WARNING/CAUTION/NOTE

Carefully read and strictly follow all Warnings and Cautions listed in this user guide. Servicing and maintenance should only be done by qualified personnel.

🔥 WARNING

- ✓ Always hold the Bracket with both hands when you manipulate it.
- ✓ Operate the bracket only as described in this user guide.
- ✓ Do not modify the bracket, or any component of Technimount system. Modifying the product can cause unpredictable operation resulting in injury to the patient or operator.
- ✓ It is the responsibility of the operator, to ensure that equipment being used with Technimount products meet the installation specifications. Injury may result if non-compatible products are used with Technimount System products.
- ✓ Do not attempt to operate, install or remove the equipment while mobile. Ensure that installation and removal of equipment is done while the vehicle is immobilized.
- Verify that the bracket is inserted correctly into the a mounting system and locked. If equipment is improperly
 installed and locked, it can cause the equipment to fall and cause injury to the patient or operator and/or damage
 to the medical equipment.
- ✓ Do not allow untrained staff to assist in the operation of the mounting system. Untrained technicians/staff can cause injury to the patient or themselves.
- ✓ Do not place additional equipment or items onto the bracket or mounts other than approved Technimount or components, as this could damage the product and may result in injury to the patient or operator.
- ✓ Operators must be able to safely lift the total weight of the bracket system and medical device.
- ✓ Do not attach restraints to the bracket frame. It may result in damage to the System and/or result in injury to the patient or operator.
- ✓ Always reposition the equipment with care, avoid any improper pushing or violent manipulations, as it may result in unbalanced equipment and may cause injury to the patient or operator and/or damage the product.
- ✓ Improper maintenance can cause injury to the patient or operator or damage the product. Maintain the bracket and mounting system as described in this user guide. Use only Technimount approved parts and maintenance procedures. Using unapproved parts and procedures could cause unpredictable operation and/or injury and will void the product warranty.
- ✓ Failure to properly clean or dispose of corrosive products will increase the risk of premature damage and may cause injury to the patient or operator.
- ✓ Any installation on a surface, wall or the structure of the vehicle must be validated or inspected in order to ensure it maintains the integrity of the vehicle.
- ✓ Do not put hands or fingers on top of the medical device when pivoting the handle to install or remove it from its bracket to avoid injury.

WARNING/CAUTION/NOTE (CONTINUED)

- ✓ Only certified technical personnel familiar with the bracket installation and use should manipulate it. Always refer to Technimount's user guides for all instructions for installing and using any Technimount mounting system.
- ✓ Regulary inspect all of the equipment's components for any issue and loose screws, bolts and nuts.
- ✓ Never install the mount into or onto other similar mounting systems or brackets without written confirmation by Technimount EMS as these different systems may be from other brands or models and may not be compatible with Technimount systems.

<u>NOTE</u>

- ✓ Some cleaning products are corrosive in nature and may cause damage to the product if used improperly. If such products are used to clean Technimount equipment, it must be rinsed with clean water and thoroughly dried following the cleaning. Failure to properly rinse and dry the Mounting Systems will leave a corrosive residue on the surface, possibly causing premature corrosion of critical components.
- ✓ When ordering a bracket, it is important to mention which mounting system you have, as there are different systems for different EMS applications, e.g., EMS ground mounting systems.
- ✓ A maintenance program should be established for all Technimount equipment. Preventive maintenance may need to be performed more frequently, based on the level of use of the product. Pay close attention to all safety features (i.e.: screws, quick release mechanisms, and attachment points).
- ✓ Failure to use authorized parts, lubricants, etc., could damage the equipment and will void the warranty of the product.
- ✓ This user guide should be considered a permanent part of the Bracket and should remain with the product even if the equipment is subsequently sold.
- ✓ The Fluid Bag (IV) Pole is only meant to be used for the temporary transfer between the ambulance and hospital. This pole CANNOT be used inside the ambulance during EMS transport.
- ✓ Technimount continually seeks advancements in product design and quality. Therefore, while this user guide contains the most current product information available at the time of printing, there may contain minor differences between your mounting system and this user guide. If you have any questions, please contact Customer Service at customerservice@technimount.com, Technical Support at techsupport@technimount.com, or +1 888.639.2758.

REMOVING THE PACKAGING FOR INSTALLATION

- 1. Unpack boxes and check all items.
- 2. Ensure that all shipping and packaging materials have been properly removed from the product(s) prior to installation.
- 3. Identify all of the product components and hardware prior to starting the installation.
- 4. The Bracket System must work properly before being put into service.
- 5. Refer to the identification of components at the beginning of this user guide if needed.

TOOLS REQUIRED FOR INSTALLATION


No tools are required for installation. If you have any questions regarding the installation, or need assistance, please contact Technical Support at techsupport@technimount.com.

LIST OF MATERIALS


✓ Bracket Pro Serie 120-GR3

INSTALLATION OF THE BAXTER PUMPS ONTO THE BRACKET


1. Place the bracket on a stable surface for installation.

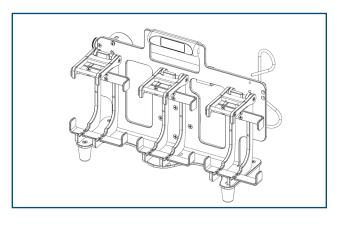

2. Pull the Red Quick Release Mechanism towards you and lift the top part of the holder.

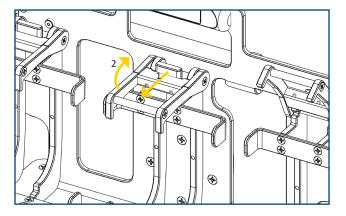

3. Insert the Baxter Pump into the holder.

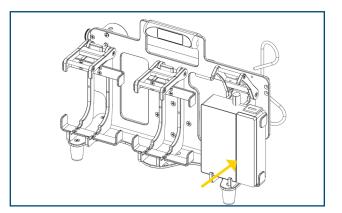


Return To Table of Contents

INSTALLATION OF THE BAXTER PUMPS ONTO THE BRACKET (CONTINUED)


4. Lower the top part of the holder over the pump until you hear the click sound.

NOTE:


Make sure the pump is securely fastened in its holder.

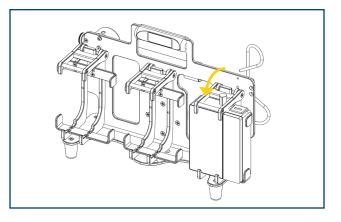

5. Repeat steps 2 to 4 to install up to three pumps onto the bracket.

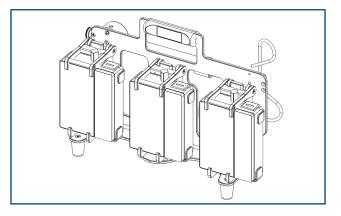


6. Once properly locked the Baxter pumps are ready for EMS transport.

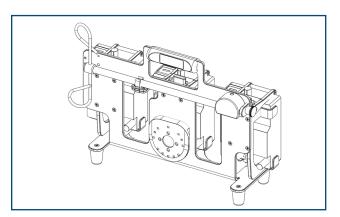

INSTALLATION OF THE IV POLE


1. Pivot the IV Pole to a vertical position, until you hear the click sound.

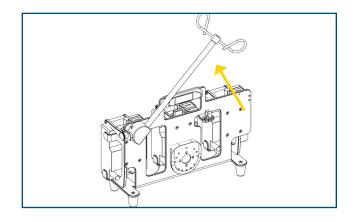

2. The IV Pole is now ready to be used with IV bags.

🚺 WARNING

✓ The IV Pole is only for temporary transport from hospital to ambulance. Do not use the IV Pole during the EMS transport.

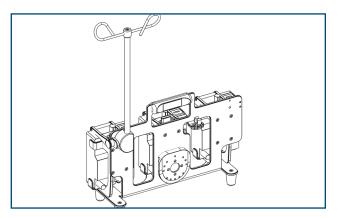

KITS AND OTHER OPTIONS

DESCRIPTION	<u>PART NUMBER</u>
Bracket Pro Serie 120-GR3	1500-10-BXSGM-GR3

WARNING

Do not modify any component of this system. Modifying the products can cause unpredictable operation resulting in injury to the patient or operator.

<u>NOTE</u>

Technimount reserves the right to change Part Numbers and Products without notice. Please refer to Customer Service at customerservice@technimount.com to ensure product part number availability.

For any replacement parts or repair, please contact Technical Support at techsupport@technimount.com.

CLEANING THE BRACKET SYSTEM

CLEANING PROCESS

🔥 WARNING

Follow your EMS service protocol or medical device's manufacturer user guide for the recommended cleaning procedures of your medical devices. The cleaning procedures below do NOT provide recommendations for the maintenance of other medical devices. The following cleaning guidelines consider the Technimount mounting system and its components.

The Bracket can be cleaned by using a pressure washer. The bracket may show some signs of oxidation or discoloration from continuous washing, however, the cot / stretcher's performance or functionality will not be affected due to power washing if cleaning instructions are properly followed.

The material used to manufacture the Bracket is high-grade aluminum. Although very durable and resistant to corrosion, high levels of sodium or a high concentration of sodium or acid may prematurely corrode the product. Always rinse with soft soap and water if exposed.

- ✓ Use of a power washer can accelerate removal of contaminants collected during the use of the product.
- ✓ Rinse with clean water.
- ✓ Towel dry all components.
- ✓ Allow all other components to air dry.
- ✓ Avoid over saturation and ensure that the product does not stay wet longer than the cleaner's manufacturer guidelines for proper disinfecting.

🔥 WARNING

- ✓ When cleaning, always use appropriate personal protection equipment (PPE) based on established protocols (e.g., gloves, eyewear, etc.).
- ✓ Refer to the product Safety Data Sheets (SDS) for chemical information or handling, storage and emergency measures in case of accident.

A CAUTION

- ✓ Do not steam clean or use ultrasonic cleaners on the system or any of its components.
- ✓ Do not immerse the metal parts/components in water.
- ✓ Maximum water temperature should not exceed 180°F / 82° C.
- ✓ Maximum water pressure should not exceed 1500 psi / 103.5 BAR. If a pressure washer is being used to clean the unit, the pressure nozzle must be kept a minimum of 24 in. (61 cm) from the unit.

CLEANING THE BRACKET SYSTEM (CONTINUED)

CLEANING SOLUTIONS

Phenolic type or quaternary type disinfectants can be used (excluding Virex[®] TB). Iodophor type disinfectants, Peracetic Acid, Chlorine, and especially Hydrogen Peroxide are not recommended for use because staining and corrosion may result.

Suggested cleaners for the Bracket:

- ✓ Quaternary Cleaners (active ingredient ammonium chloride)
- ✓ Phenolic Cleaners (active ingredient o-phenyl phenol)
- ✓ Chlorinated Bleach Solution (3.25% less than 1-part bleach to 100 parts water)

A WARNING

- ✓ Some cleaning products are corrosive in nature and may cause damage to the product if used improperly.
- ✓ If the products described are used to clean the equipment, the Bracket and components must be rinsed with clean water and thoroughly dried following cleaning. Failure to properly rinse and dry the system will leave a corrosive residue on the surface of the product, possibly causing premature corrosion of critical components.

REMOVAL OF IODINE COMPOUNDS

Use a solution of 0.13 oz / 3.70 ml of Sodium Thiosulfate in 1 pt / 0.5 L of warm water to clean the stained area. Clean as soon as possible after staining occurs. If stains are not immediately removed, allow solution to soak or stand on the surface. Thoroughly rinse surfaces with clean water and allow to air dry before returning unit to service.

✓ Failure to properly clean contaminated parts or components will increase the risk of exposure to blood borne pathogens and may cause injury to the patient or the operator.

PREVENTIVE MAINTENANCE

A preventive and regular maintenance program should be established for all Technimount equipment. Preventive maintenance may be required more frequently based on the usage level of the product. The Bracket requires regular preventative maintenance. Establish and follow a preventive maintenance schedule and keep records of preventive maintenance activities (see maintenance log in this user guide).

🔔 CAUTION

- ✓ Close attention should be given to safety features including, but not limited to locking mechanisms and Discs.
- Improper maintenance can cause injury or damage to the product. Maintain the product as described in this user guide.

LUBRICATION

The Bracket System has been designed to operate without the need for lubrication. If you have questions, please contact Technical Support at techsupport@technimount.com.

AUTION

✓ Failure to use authorized parts, lubricants, etc. could cause damage to the cot/stretcher and will void the warranty of the product.

Return To Table of Contents

INSPECTION PROCESS AND SCHEDULE

MAINTENANCE PLAN

The following inspection routine and schedule is intended as a general guide for preventive maintenance of the Bracket. Factors such as weather, environment, geographical location, and individual usage will necessitate different maintenance. If you are unsure as to how to perform these maintenance inspections or at what interval to perform these inspections, please contact Technical Support at techsupport@technimount.com. Check each routine and replace damaged or worn out parts when necessary.

Follow the timetable below for maintenance (either in months (M) or hours (H)), in accordance with your Service's current maintenance practices and protocols.

<u>ITEM</u>	INSPECTION	<u>1 M</u> <u>OR</u> <u>2 H</u>	<u>3 M</u> OR <u>6 H</u>	<u>6 M</u> <u>OR</u> <u>12</u> <u>H</u>	<u>12</u> <u>М</u> <u>OR</u> <u>24</u> <u>Н</u>
Bracket	 ✓ Inspect Bracket Inspect the screws Inspect the Quick Release Mechanisms to ensure there are no debris or obstacles Inspect back screws Push and release the Red Quick Release Mechanisms repetedly to ensure proper functioning Pivot the IV Pole up and down to ensure proper functioning Verify Discs Verify that there is no damage or dirt on the discs and there are no loose screws The discs can be easily inserted into and removed from Micro Base ✓ Do a visual inspection for the Bracket to ensure there is no damage or chemical attack 	Х			

INSPECTION AND MAINTENANCE LOG

INSPECTION	<u>BY</u>	<u>DATE</u>	<u>TIME</u>

TRAINING LOG

	TRAINING DATE			
TRAINEE NAME	<u>BASIC</u> <u>TRAINING</u>	<u>TRAINING</u> <u>UPDATE</u>	<u>TRAINING</u> <u>METHOD</u>	

REPLACEMENT PARTS

The parts and accessories listed below are all currently available for purchase. Some of the parts illustrated in this user guide may not be individually available for purchase. Please contact Customer Service at customerservice@ technimount.com or +1.888.639.2758.

DESCRIPTION	<u>PART NUMBER</u>
IV Pole	940-00-IV2-11
IV Pole Clip	986-00-IV
Acetal Feet	923-00-78-INS
Bracket Pro Serie 120-GR3	1500-10-BXSGM-GR3

WARRANTY POLICY

This statement constitutes TECHNIMOUNT's entire warranty policy with regards to the TECHNIMOUNT Products.

TECHNIMOUNT MAKES NO OTHER WARRANTY OR REPRESENTATION NEITHER EXPRESSED NOR IMPLIED, EXCEPT AS SET FORTH HEREIN. THERE IS NO WARRANTY OF MERCHANTABILITY AND THERE ARE NO WARRANTIES OF FITNESS FOR ANY PARTICULAR PURPOSE. IN NO EVENT SHALL TECHNIMOUNT BE LIABLE HEREUNDER FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING FROM OR IN ANY MANNER RELATED TO SALES OR USE OF ANY SUCH EQUIPMENT.

TECHNIMOUNT E.M.S. Holding Inc. (TECHNIMOUNT) guarantees to the original "Purchaser" of the "Hardware" with which this "Limited Warranty" is included that the Hardware will be free from "Defects" in workmanship and materials under normal use for a "Warranty Period", one (1) year from the date that the Hardware was first purchased by the Purchaser. During the Warranty Period, the Hardware will be repaired or replaced according to the "Limited Warranty" without charge to the Purchaser for either parts or labor. The parts or products may be repaired or replaced with either new or refurbished parts. For this Limited Warranty "refurbished" means parts and products, which have been returned to factory specifications. If the Hardware is repaired or replaced within the Warranty Period, the greater of the remaining warranty period will apply or three (3) months from the date of repair/replacement. If the Hardware is repaired or replaced after the Warranty Period has expired, the Warranty Period for the repair or replacement will expire three (3) months after the date of repair or replacement.

LIMITED RESPONSIBILITY AND WARRANTY

The Limited Warranty does not apply to normal wear that should result from normal use. It does not apply when the Hardware or any component has been, disassembled, or repaired by someone not authorized by TECHNIMOUNT or if the seal has been broken. It does not cover repair or replacement of any Hardware or part thereof damaged by neglect, misuse, moisture, liquids, exposure to heat, accidents, abuse, and non-compliance with the instructions for installation and use provided with the Hardware. The Limited Warranty does not cover physical damage to the surface of the Hardware and the decision to repair, replace or refuse the coverage is final and at the sole discretion of TECHNIMOUNT, without any compensation or obligation from TECHNIMOUNT.

The hardware, or product defined as a mounting or bracket system for clipping and attaching medical equipment is specifically designed to fill these requirement. Any other use will void the warranty and TECHNIMOUNT will not be held liable on any claim if the product has been modified or adapted for use.

Technimount products are intended to retain a medical device in place in the case of a single crash impact. A Technimount product must NOT be used again if it was involved in a crash. The product MUST be replaced. If the Purchaser uses a Technimount product following a crash, it is at the Purchaser's own risk and Technimount will not be held liable.

INTERNATIONAL WARRANTY CLAUSE

This warranty reflects Canadian domestic policy. Warranty outside Canada may vary by country. Please contact Customer Service at customerservice@technimount.com for more information.

RETURN POLICY

Mounting systems and bracket systems for portable medical devices may be returned up to 60 days of receipt if:

- The product is not what was originally ordered
- The product does not meet specifications with TECHNIMOUNT's technical sheets
- The product is not compatible with the equipment on which it was to be installed

For any manufacturing defect, refer to the conditions within the Warranty Policy

PRIOR TO 30 DAYS

- Product must be undamaged and in its original packaging
- The product return request must be provided in writing and must be approved by TECHNIMOUNT prior to returning the product
- Returns will not be approved on a modified or damaged item
- Charges may apply if damaged or missing item
- Customer is responsible for a 10% restocking fee

PRIOR 45 DAYS

- Product must be unused, undamaged and in its original packaging
- The product return request must be provided in writing and it must be approved by TECHNIMOUNT prior to returning the product
- Returns will not be approved on modified or damaged item
- Charges may apply if damaged or missing items
- Customer is responsible for a 25% restocking fee

PRIOR 60 DAYS

- Product must be unused, undamaged and in its original packaging
- The product return request must be provided in writing and it must be approved by TECHNIMOUNT prior to returning the product
- Returns will not be approved on a modified or damaged item
- Charges may apply if damaged or missing items
- Customer is responsible for a 30% restocking fee

RETURN AUTHORIZATION

TECHNIMOUNT's customer service is responsible for approving returns and will provide a Return Merchandise Authorization (RMA) number to be printed on any returned merchandise. TECHNIMOUNT reserves the right to charge shipping and restocking fees on returned items. SPECIAL, MODIFIED, OR DISCONTINUED ITEMS ARE NOT SUBJECT TO RETURN.

DAMAGED MERCHANDISE

ICC Regulations require that claims for damaged merchandise must be made with the carrier within fifteen (15) days of receiving merchandise. DO NOT ACCEPT DAMAGED SHIPMENTS UNLESS SUCH DAMAGE IS NOTED ON THE DELIVERY RECEIPT AT THE TIME OF RECEIPT. Upon prompt notification, TECHNIMOUNT will file a freight claim with the appropriate carrier for damages incurred. Claims will be limited in amount to the actual replacement cost. In the event that this information is not received by TECHNIMOUNT within the fifteen (15) day period following the delivery of the merchandise, or the damage was not noted on the delivery receipt at the time of receipt, the customer will be responsible for payment of the original invoice in full.

Note: Claims for any short or broken shipment must be made within thirty (30) days of invoice.

CLAIM PROCESS

Please follow the claim procedure below to return a defective product: Download the form at https://www.technimount.com/wp-content/uploads/2021/12/Technimount-RMA-EMS-FOR-03-03.pdf.

REQUIRED INFORMATION

- Serial number
- Invoice number
- Identification of the issue
- Upload the pictures of the issue
- Submit the form

A confirmation of the receipt of the claim will be sent to you within 2 business days. If you have not received a confirmation e-mail by then, please contact Technical Support at techsupport@technimount.com.

If the RMA request is approved, TECHNIMOUNT will provide you with an RMA number for your claim. We will also include instructions for the replacement of your product. No product return will be accepted without the RMA number labeled on the outside of the box being returned.

FINDINGS AND CONCLUSION

- If following an investigation, we find that our product is defective, TECHNIMOUNT will take corrective actions and close the claim.
- If following an investigation, we find that our product is NOT defective (misuse or abuse of the product) the product will not be covered by the warranty. Details of our findings and conclusions will be provided to you.

QUESTIONS ABOUT OUR POLICY

If you have any questions regarding our return policy, please contact Customer Service at customerservice@ technimount.com.



SAFETY AND FLEXIBILITY WHERE IT MATTERS MOST

TECHNIMOUNT E.M.S. HOLDING INC. 3770 Jean Marchand Street, Suite 100-C Quebec (QC) G2C 1Y6 Canada T + 1 581.700.6613 TF + 1 888.639.2758 info@technimount.com technimount.com

